

URIT-12 Hemoglobin Meter



- **FAST hemoglobin and HCT test within 10 seconds**
- **Accurate & Reliable Result**
- **Easy 3-step operation**

Specifications

Parameter: Hemoglobin, HCT (Hematocrit)

Principle: Optical reflectance

Sample: Capillary or venous whole blood (13~15 ul)

Strip: H12 Hemoglobin Test Strip

Speed: ≤ 10 seconds

Measuring Range: 4.0g/dL ~ 24.0g/dL(g/L optional)

Memory: 250 test results

Quality Control: HQ-A Hemoglonbin control solution

Calibration: Factory calibrated according to ICSH

Automatization: Self-checking, auto-judging and displaying malfunction

Power: DC 6V (Two CR2032 Batteries)



Dimension: 102mm × 50mm × 19mm

URIT-12 Hemoglobin Meter



Accuracy: accuracy ≥ 96%, the correlation is very good in the comparison between URIT-12 and ICSH method.

Precision: CV < 5%, testing samples including high, medium & low concentration, the CV of 10 repeated test results is 1.8% 2.2% 2.7% respectively.

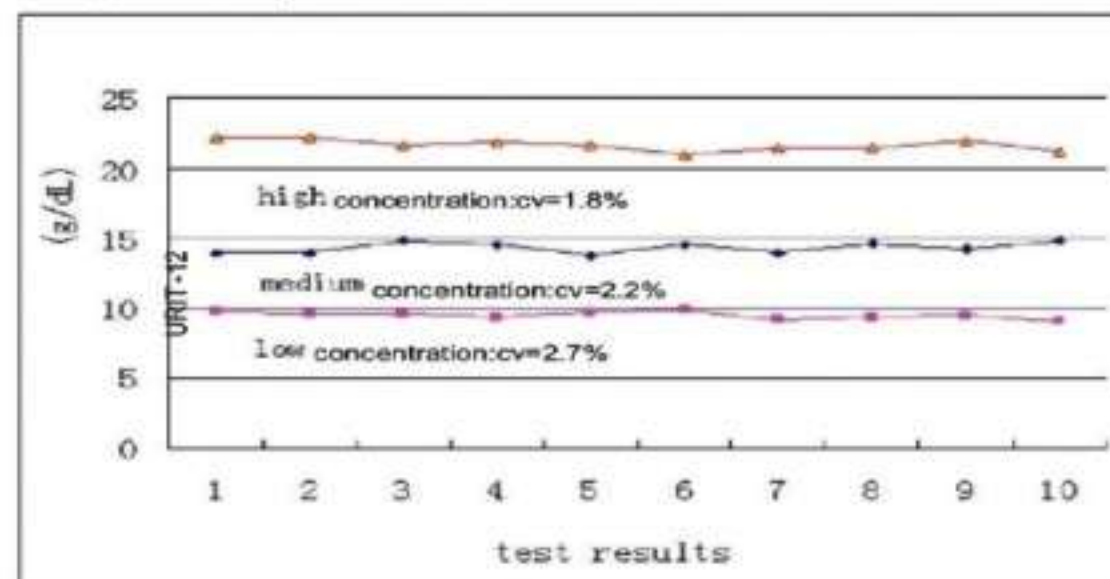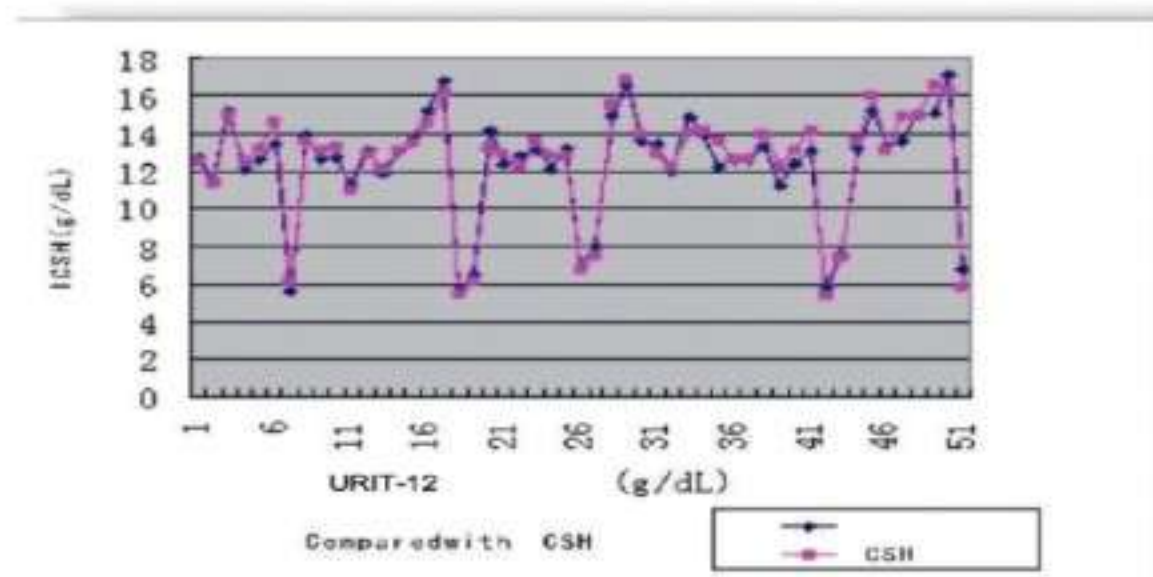

Operation



STEP 1

Turn on the meter, insert the test strip



STEP 2

Apply blood sample to the test strip



STEP 3

Read the test result

ACCUREX

HEAD OFFICE

212, Udyog Mandir No. 1, 7-C, Bhagoji Keer Marg, Mahim (W),
Mumbai - 400016, Maharashtra, India

Customer Care: +91 7400 453 000

www.accurex.net